
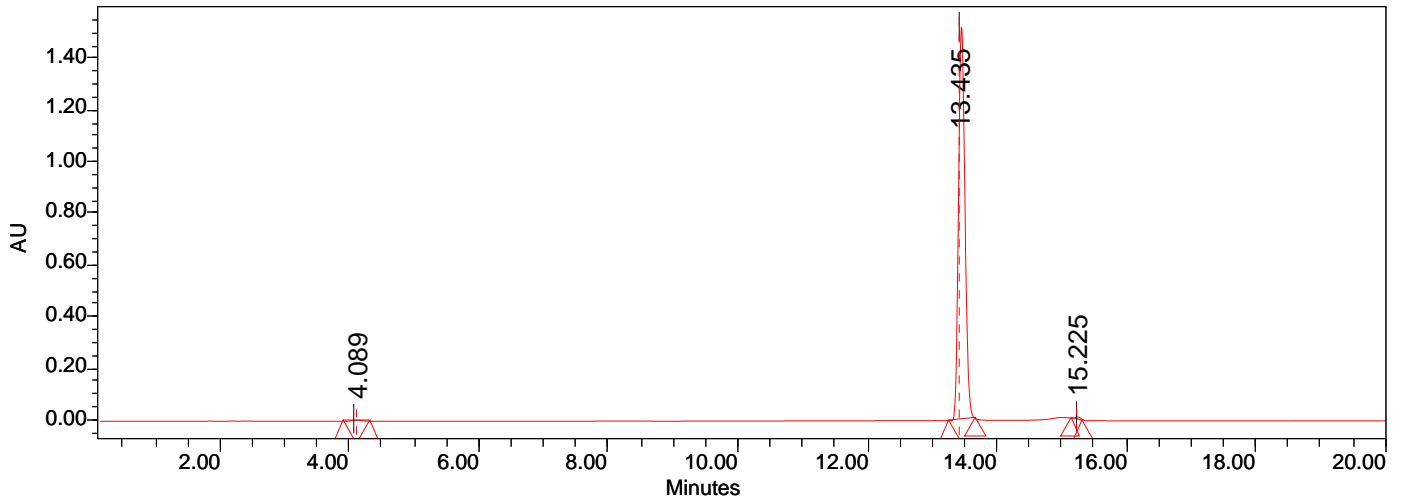


Sample Name: MT-524-2

Injection Id: 1263

Result Id 4154

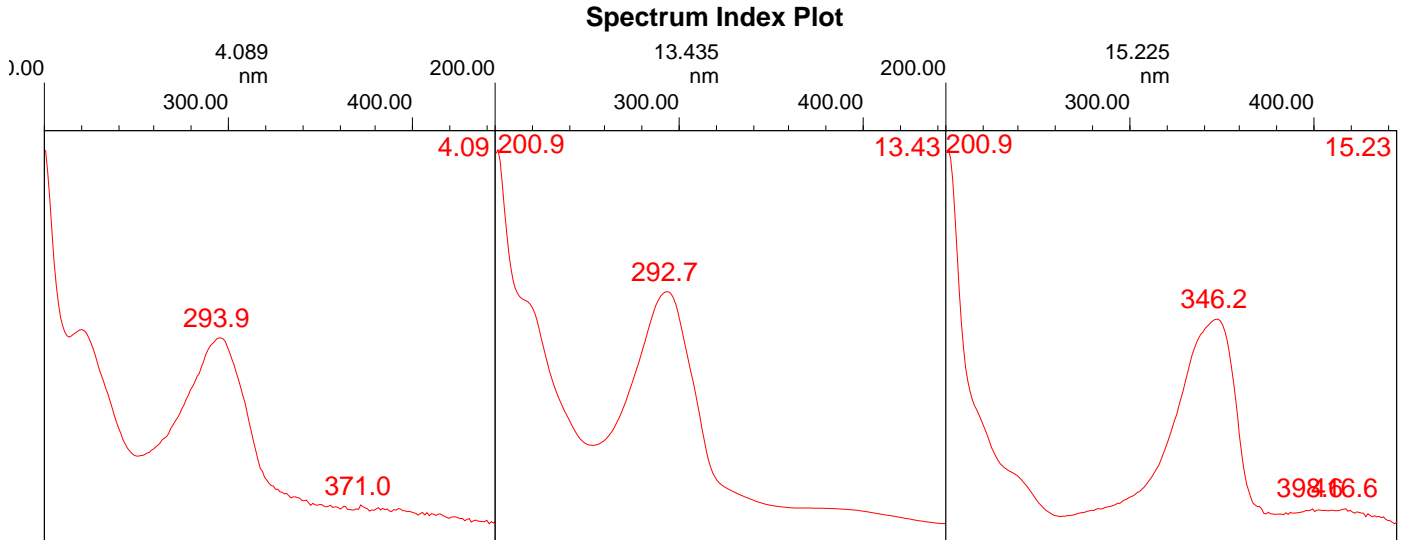


Channel Name: MaxPlot 220.0 to 450.0nm

Peak Results


Name	RT	Area	Height	Amount	Units	% Area	% Height	Int Type	Purity1 Angle	Purity1 Threshold	Purity1 Flag
1	4.089	38105	3802			0.36	0.25	bb	0.485	0.554	No
2	13.435	10545766	1521420			99.14	99.18	BB	0.212	2.196	No
3	15.225	53262	8701			0.50	0.57	bb	1.161	0.409	Yes

Purity Plot

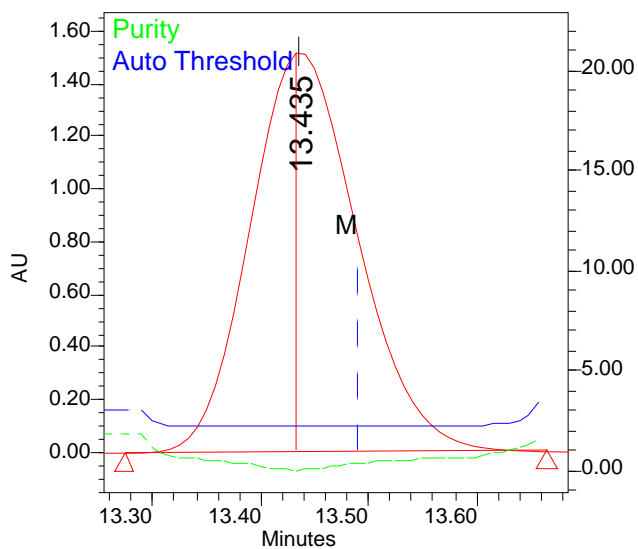

PA: 0.212 TH: 2.196

— Peak:
- - - Purity
- - - Noise

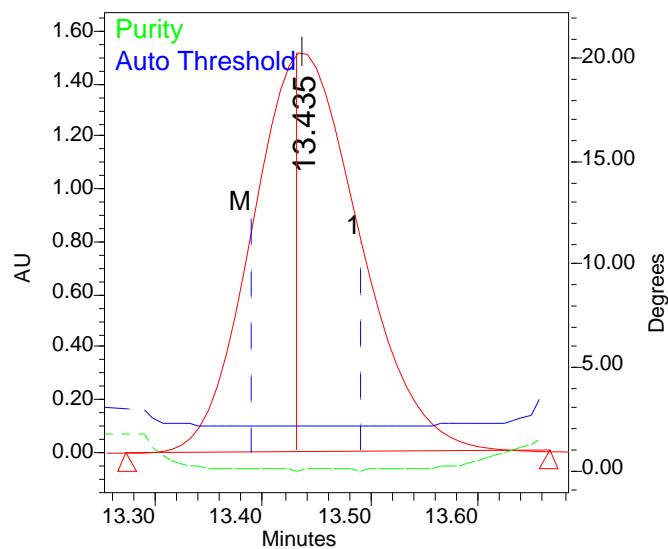

PA: 0.022 TH: 2.196

Injection Volume: 10.00 ul

Run Time: 20.00 Minutes

Column: Phenomenex Synergi Polar-RP 4µ

Column Size: 4.6 mm x 150 mm

Temperature: ambient

Solvents


	Solvent_C	Solvent_D
1	CH3CN, 3%H2O	H2O, 0.1%TFA, 3%CH3CN

Instrument Method: PDA gradient 30to90

Stored: 3/28/01 10:28:12 AM

W600 Gradient Table

	Time	Flow	%A	%B	%C	%D	Curve
1		1.00	0.0	0.0	30.0	70.0	
2	3.00	1.00	0.0	0.0	30.0	70.0	6
3	15.00	1.00	0.0	0.0	90.0	10.0	6
4	20.00	1.00	0.0	0.0	30.0	70.0	11
5	50.00	0.20	0.0	0.0	30.0	70.0	11

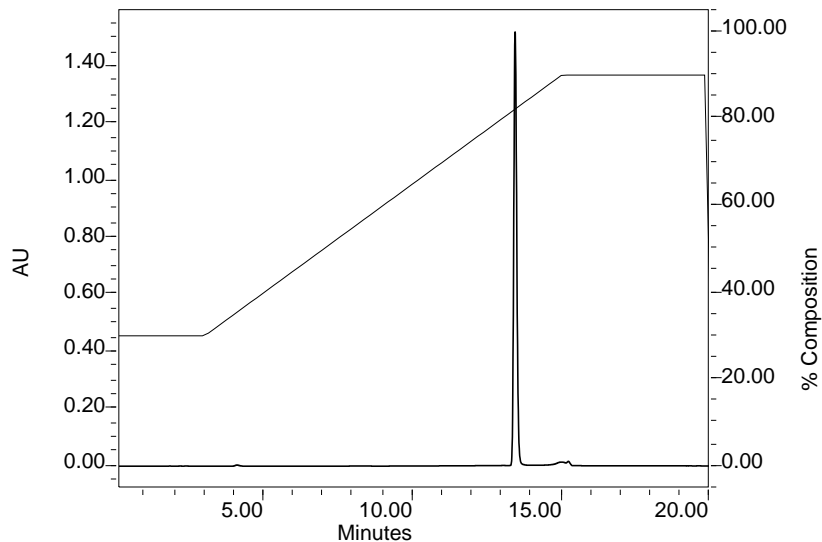

Date Acquired: 3/28/01 10:29:54 AM

Date Processed: 7/27/01 12:52:46 PM